

# X-RAY ILLUMINATOR, 3792GF (ONE-BANK), 3793GF (TWO-BANK), 3795GF (THREE-BANK): INSTALLATION AND OPERATION INSTRUCTIONS

## PLEASE SAVE THESE INSTRUCTIONS FOR FUTURE USE

Installation tools and supplies: Level, screwdriver, one  $\#10 \times 1^{-1/2}$ " sheet metal screw, one #10 drywall anchor and screw

Fuse replacement: Phillips screwdriver

**⚠ WARNING: Important! Read and understand these instructions before installing the** 

X-Ray Illuminator. If you do not understand any part of these instructions, contact your medical supply distributor for direction in the use of this product. If the X-Ray Illuminator is not properly installed, personal injury and/or

damage to the X-Ray Illuminator could result.

**NOT** use substitute parts.

 $\triangle$  WARNING: GF Health Products, Inc. assumes no responsibility for any damage or injury

caused by improper installation or use of this product.

**INSTALLATION (ON WALL OR TABLE)** 

stepped on, tripped over, or otherwise subjected to damage or stress. Do not


use this unit with an extension cord.

### **INSTALLATION ON WALL**

sonal injury.

1. The one-bank X-Ray Illuminator is shown at right. Open the front cover of the X-Ray Illuminator to access the mounting slots in the back wall: Grasp the upper corners at the **OPEN** labels and pull forward. Rotate the front of the X-Ray Illuminator forward carefully and let it hang.

2. Find the wall stud where you will mount one side of the X-Ray Illuminator (see preceding warning). Hold the X-Ray Illuminator, with level on top, up to the wall to find the desired mounting height. Place one of the mounting slots directly over the wall stud.

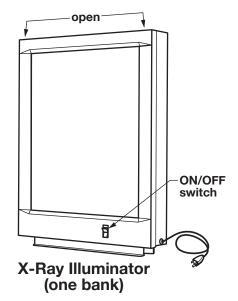

GF0700102RevB07


- 3. Mark in the center of both slots, at the locations shown in the picture at right. Remove the X-Ray Illuminator.
- 4. Install the sheet metal screw in the marked location in the wall stud. Use screwdriver to secure, but not completely.
- 5. Install the drywall anchor and screw in the other marked slot (per the drywall anchor and screw mounting instructions). Use screwdriver to secure, but not completely.
- 6. Lift the X-Ray Illuminator and place the back flat against the wall with large round holes over screw heads. Slide X-Ray Illuminator down carefully so that tops of slots are resting on screws.
- 7. Use the screwdriver to tighten both screws securely.



mounting screw

install illuminator

on mounting screws



over mounting screws

-install screw at x-

mounting slot

## **INSTALLATION ON TABLE**

Set the X-Ray Illuminator on a sturdy table, ensuring that its base is flat and stable.

#### **OPERATION**

⚠ WARNING: This device is equipped with a three-prong (grounding) plug for protection against possible shock hazard. Plug only into a properly grounded threeprong wall receptacle.

- 1. Plug the X-Ray Illuminator into a properly grounded power outlet.
- 2. Turn the X-Ray Illuminator ON by pressing the ON/OFF switch on front of unit.
- 3. Slide X-Ray up into holder on top front of unit.

## **MAINTENANCE**

bulbs or fuse; otherwise, shock or electrocution could occur.

Replacing fluorescent tubes: Replace with T-8 15W Medium Bi-Pin 18" (one-bank requires three tubes, two-bank requires six tubes, three-bank requires nine tubes).

**Replacing fuse**: Replace fuse with same size and type. Use screwdriver to remove fuse holder. Remove old fuse and replace with new fuse. Replace fuse holder. Use screwdriver to secure.

#### WARRANTY

GF Health Products, Inc. warrants the Grafco X-Ray Illuminator for a period of ninety days for defects in workmanship and materials. During the warranty period, defective items will be repaired or replaced at manufacturer's option at no charge.



www.grahamfield.com

GF, Graham-Field and Grafco are registered trademarks of GF Health Products, Inc.

© GF Health Products, Inc. • 2935 Northeast Parkway • Atlanta, GA 30360 • tel 800-347-5678 • fax 800-721-0601 • www.grahamfield.com