





HSP-1007-05 (Standard 4")  
600C-100705 (Hausted Clinical Comfort 5")

Stryker®  
TRANSPORT 720/721 24" LITTER

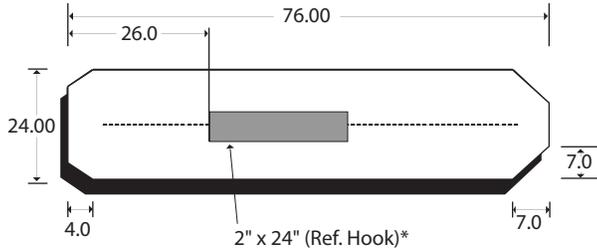


HSP-1007-06 (Standard 4")  
600C-100706 (Hausted Clinical Comfort 5")

Hill-Rom®  
ELECTRIC (P8020)  
TRANSPORT 720/721 24" LITTER

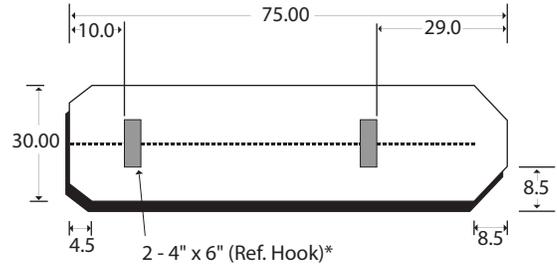


HSP-1007-07 (Standard 4")  
600C-100707 (Hausted Clinical Comfort 5")

Hill-Rom®  
GPS 880/881/882/883

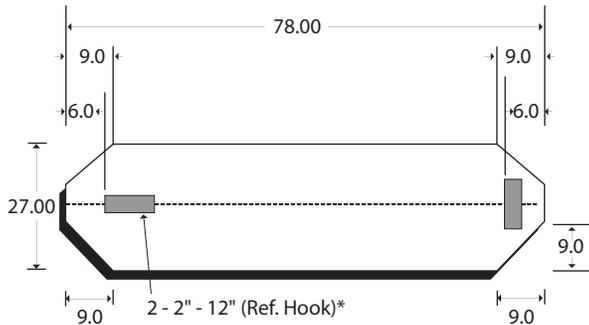


HSP-1007-08 (Standard 4")  
600C-100708 (Hausted Clinical Comfort 5")

Hill-Rom®  
GPS 885/886

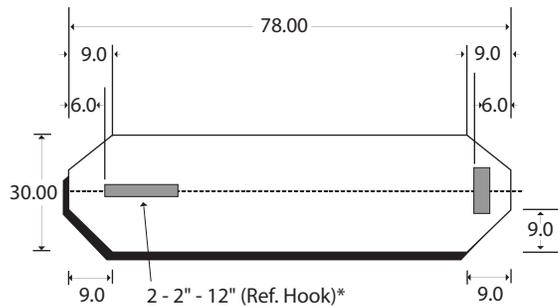


HSP-1007-09 (Standard 4")  
600C-100709 (Hausted Clinical Comfort 5")

Hill-Rom®  
PROCEDURAL (P8000)  
TRANSPORT (P8005) 26" PATIENT SURFACE  
TRAUMA (P8040)

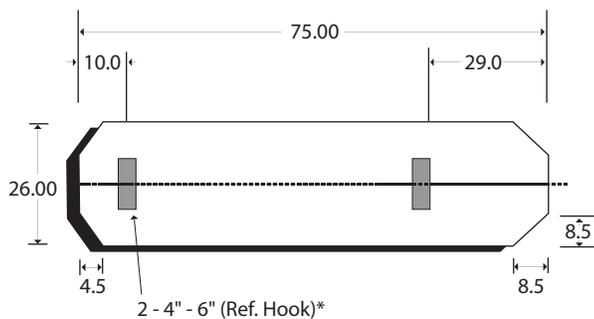

HSP-1007-10 (Standard 4")  
600C-100710 (Hausted Clinical Comfort 5")

Hill-Rom®  
SURGICAL (P8010)

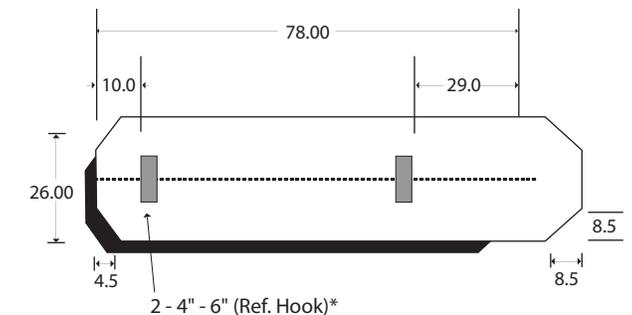

Follow us on:



Drawings are not to scale. GF Health Products, Inc. is not responsible for typographical errors. All design details, illustrations, specifications, packaging and warranties contained in this literature are based on the latest product information available at the time of printing and are subject to change. The most current product information can be found online at [www.grahamfield.com](http://www.grahamfield.com). 2016 © GF Health Products, Inc.

\*Location of hook/loop on bottom of pad may not match location of attachment point on stretcher. Make sure pad is securely attached to stretcher to avoid injury.