

- ⚠ **WARNING: Important! Read and understand these instructions before assembling or using the Physician Exam Stool. If you do not understand any part of these warnings, cautions or instructions, contact a healthcare professional for direction in the use of this product. If the Physician Exam Stool is not properly assembled and used, personal injury and damage to the Physician Exam Stool could result.**
- ⚠ **WARNING: If components are damaged or missing, contact your dealer immediately. DO NOT use substitute parts. Use only Lumex replacement parts. Non-Lumex replacement parts could cause personal injury and damage to the Physician Exam Stool.**
- ⚠ **WARNING: 900 Series Physician Exam Stool maximum weight capacity is 350 lb (159.79 kg), EVENLY DISTRIBUTED.**
- ⚠ **WARNING: GF Health Products, Inc. assumes no responsibility for any damage or injury caused by improper installation or use of this product.**

INTENDED USE

The Physician Stool is intended as a medical-room or clinical setting stool for professional use only.



9501 Physician Stool

UNPACKING



Check for any obvious damage to the carton or contents (after unpacking). If damage is evident, immediately notify the carrier and Lumex.

Open the box and carefully remove the back, base, seat, and foot-ring and place each component on plastic or in protected area. Then, remove any other contents of the box carefully.

STOOL ASSEMBLY

Tools required: None

Basic Stool Assembly

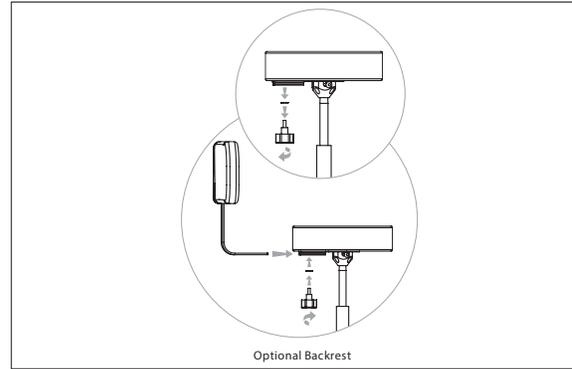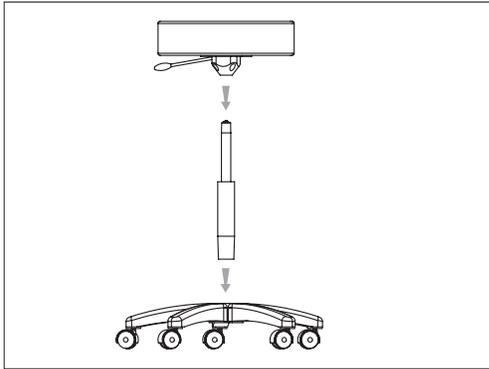

1. Remove casters from the bag, and turn over base of stool.
2. Firmly press each caster to the base of the stool.
3. Flip the base over so that the casters are touching the floor.
4. Position the foot-ring on the gas cylinder at desired height, hold bottom of the plastic hub with one hand and the outer ring with the other hand. Turn clockwise to tighten foot-ring.
5. Unwrap the gas cylinder from its plastic covering.
6. Place the piston's flat part down, notice the green gas cylinder will be visible and not attached to base.
7. Finally align green gas cylinder with the center of the seat hole and attach.


Optional Backrest

In order to attach the seat back to the stool, flip the seat over to the side and find the knob for the seat back. Unscrew knob then attach the back and tightly screw knob back on.

⚠ WARNING: Check the fit and tightness frequently of all fasteners to ensure that the Physician Exam Stool is securely assembled.

Height Adjustment

Pull up on lever to raise height of stool and push down on lever to lower height of stool.

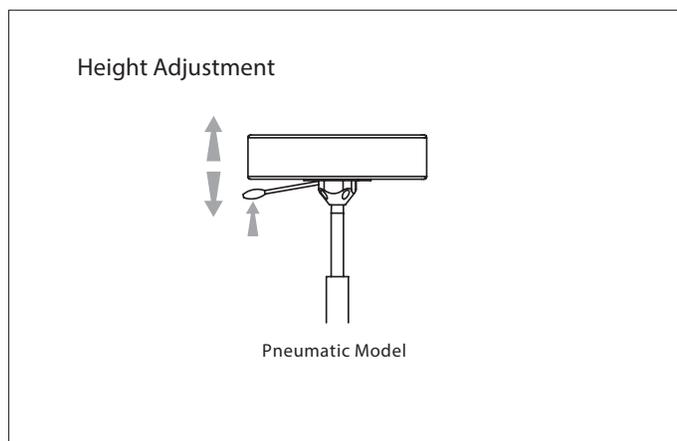

OPERATION

- ⚠ **WARNING: Ensure the Physician Exam Stool is securely assembled as previously described before each use. Monitor patient to ensure Physician Exam Stool DOES NOT adversely affect patient in any way. If so, discontinue use immediately.**

CARE AND MAINTENANCE

Cleaning and Disinfection

- ⚠ **WARNING: Check the Physician Exam Stool before each use for signs of damage. If damage is found, DO NOT use the Physician Exam Stool. Contact Lumex immediately.**

To clean Physician Exam Stool, hand wash gently with warm water and a mild soap or detergent, rinse with clear water, and air dry.

To disinfect Physician Exam Stool, use a diluted solution of 10% (or less) household bleach containing 5.25% sodium hypochlorite, rinse with clear water, and air dry.

- ▲ **NOTICE: DO NOT use abrasive cleaners or scouring pads on any part of the Physician Exam Stool.**

- ⚠ **WARNING: Inspect all components periodically and replace as needed.**

Every three months

- Check back to ensure screws are tight; if not, tighten.

Upholstery maintenance and stain removal

- Ordinary dirt: wash with warm water and a mild soap or detergent.
- Stubborn dirt: using a soft bristle brush, wash with warm water and a mild soap or detergent.
- Ground-in dirt: scrub with powdered cleanser or similar detergent.
- Chewing gum: scrape carefully; remove with kerosene or naphtha.
- Nail polish and remover: blot immediately to prevent damage.
- Ball point pen: blot immediately with a white cloth dampened in water or mineral oil.
- Paint, shoe polish, heel marks: remove immediately! Use a white cloth dampened in kerosene, naphtha or turpentine. Do not use paint remover or liquid brush cleaners.
- Tars, asphalt, creosote: remove to prevent staining. Clean area with kerosene or naphtha.

- ⚠ **WARNING: When using kerosene or naphtha, do so in a well ventilated area and keep it away from fire, flame, and chair occupant.**

- Waxing and refinishing: improves wearability. Use any quality paste wax.

LIMITED WARRANTY

SCOPE OF WARRANTY

GF Health Products, Inc. ("GF") warrants to the original purchaser only that it will replace or repair components, at GF's sole discretion, that are defective in material or workmanship under normal use and service. All warranties are conditioned upon the proper use of the products strictly in accordance with good commercial practice and applicable GF instructions and manuals, including proper use and maintenance. To the extent that a component is warranted by a third party, GF conveys all of its rights under that warranty to the original purchaser, to the extent permitted. This limited warranty shall only apply to defects that are reported to GF's customer service team within the applicable warranty period and which, upon examination by GF or its authorized representative, prove to be a warranty item. This limited warranty is not transferable. Within the guidelines set forth in this document, the following components are warranted for the time period set forth below:

Components *

Frame:.....	5 years
Mechanical Components:	3 years
Original and Replacement Upholstered Tops †:	1 year
Replacement Parts ‡:.....	90 days

* Labor is not included in the warranty.

† Upholstery is only warranted on material supplied by GF.

‡ The warranty period is as designated above. If a part is replaced under warranty, the original warranty period will not be affected. All other replacement parts will be subject to the warranty period specified.

The applicable warranty period shall commence from date of shipment to the original customer, unless there is an expiration date on the component in which case the warranty shall expire on the earlier of warranty period or the expiration date.

OBTAINING WARRANTY SERVICE

This limited warranty shall only apply to defects that are reported to the Distributor from whom the Customer purchased the product within the applicable warranty period. If there is not a Distributor, you must contact GF directly by calling 1.336.884.4096, or by e-mailing a request to GF@grahamfield.com. Specific directions will be provided by the Customer Service Representative. Failure to abide by the specific directions will result in denial of the warranty claim.

The warranty does not cover and GF shall not be liable for the following:

- 1) Defects, damage, or other conditions caused, in whole or in part, by misuse, abuse, negligence, alteration, accident, freight damage, tampering or failure to seek and obtain repair or replacement in a timely manner;
- 2) Products which are not installed, used, or properly cleaned and maintained as required in the official manual for the applicable product;
- 3) Products considered to be of a non-durable nature including, but not limited to: tips, casters, filters, fuses, gaskets, lubricants, and charts;
- 4) Accessories or parts not provided by GF;
- 5) Matching of color, grain or texture except to commercially acceptable standards;
- 6) Changes in color caused by natural or artificial light;
- 7) Charges by anyone for adjustments, repairs, replacement parts, installation or other work performed upon or in connection with such products which are not expressly authorized in writing, in advance, by GF;
- 8) Any labor or shipping charges incurred in the replacement part installation or repair;
- 9) Costs and expenses of regular maintenance and cleaning; and
- 10) Representations and warranties made by any person or entity other than GF.

ENTIRE WARRANTY, EXCLUSIVE REMEDY AND CONSEQUENTIAL DAMAGES DISCLAIMER

THIS WARRANTY IS GF'S ONLY WARRANTY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED. GF MAKES NO IMPLIED WARRANTIES OF ANY KIND INCLUDING ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. IF ANY MODEL OR SAMPLE WAS SHOWN TO THE CUSTOMER, SUCH MODEL OR SAMPLE WAS USED MERELY TO ILLUSTRATE THE GENERAL TYPE AND QUALITY OF THE PRODUCT AND NOT TO REPRESENT THAT THE PRODUCT WOULD NECESSARILY CONFORM TO THE MODEL OR SAMPLE IN ALL RESPECTS. THIS WARRANTY IS LIMITED TO THE REPAIR OR REPLACEMENT OF THE DEFECTIVE PARTS. GF SHALL NOT BE LIABLE FOR AND HEREBY DISCLAIMS ANY DIRECT, SPECIAL, INDIRECT, INCIDENTAL, EXEMPLARY OR CONSEQUENTIAL DAMAGES, INCLUDING, BUT NOT LIMITED TO: DAMAGES FOR LOSS OF PROFITS OR INCOME, LOSS OF USE, DOWNTIME, COVER, OR EMPLOYEE OR INDEPENDENT CONTRACTOR WAGES, PAYMENTS AND BENEFITS. CERTAIN STATES MAY CONFER ADDITIONAL RIGHTS REGARDING WARRANTIES AND IN THOSE STATES GF'S LIABILITY AND THE LIABILITY OF GF'S SUPPLIERS, SHALL BE LIMITED TO THE FULLEST EXTENT PERMITTED BY LAW.

The warranties contained herein, together with GF's current Terms and Conditions, contain all the representations and warranties with respect to the subject matter of this document, and supersede all prior negotiations, agreements and understandings with respect thereto. The recipient of this document hereby acknowledges and represents that it has not relied on any representation, assertion, guarantee, warranty, collateral contract or other assurance, except those set out in this document.

For additional information on these products or this warranty, please contact an GF Customer Service Representative.

NOTES:

- 1) Additional terms and conditions may apply. See GF's General Terms and Conditions on its website and the specific warranties, which may accompany the specific product.
- 2) Freight claims must be notated on the appropriate shipping documents and must be made with immediacy. International, federal and state regulations govern specific requirements for freight claims. Failure to abide by those regulations may result in a denial of the freight claim. GF will assist you in filing the freight claim.
- 3) Claims for any short shipment must be made within three (3) days of the invoice date.

LUMEX®
by graham-field

Manufactured By:

GF Health Products, Inc.
One Graham-Field Way, Atlanta, GA 30340
Made in USA



+1 770.368.4700

Information contained herein is subject to change without notice.
The most current and complete product information can be found on our website.
www.grahamfield.com

graham
field

© 2024, GF Health Products, Inc. All Rights Reserved.
Lumex is a registered trademark of GF Health Products, Inc.

LX_GF2400159-INS-LAB-RevA24